



Optical Coherence Tomography


RS-3000 Advance / Lite



THE ART OF EYE CARE


Wide Area and High Definition OCT with SLO Tracing


12 mm wide horizontal scan available with the RS-3000 Advance allows detailed observation of the vitreous body, retina, and choroid from the macula to optic disc in a single image.

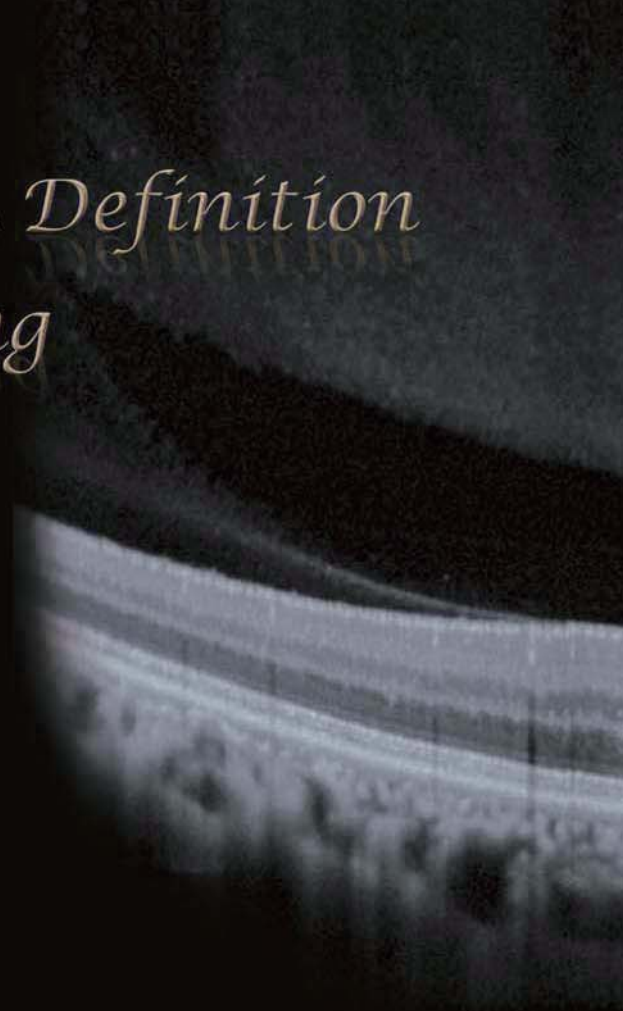

Selectable OCT Sensitivity

Selecting the OCT sensitivity based on ocular pathology allows image capture with higher definition or at high speed. Ultra fine, fine, and regular sensitivities are available for the RS-3000 Advance and fine and regular sensitivities are available for the RS-3000 Lite. Ultra fine and fine sensitivities are used to capture high definition images and regular sensitivity is used to capture images at high speed.


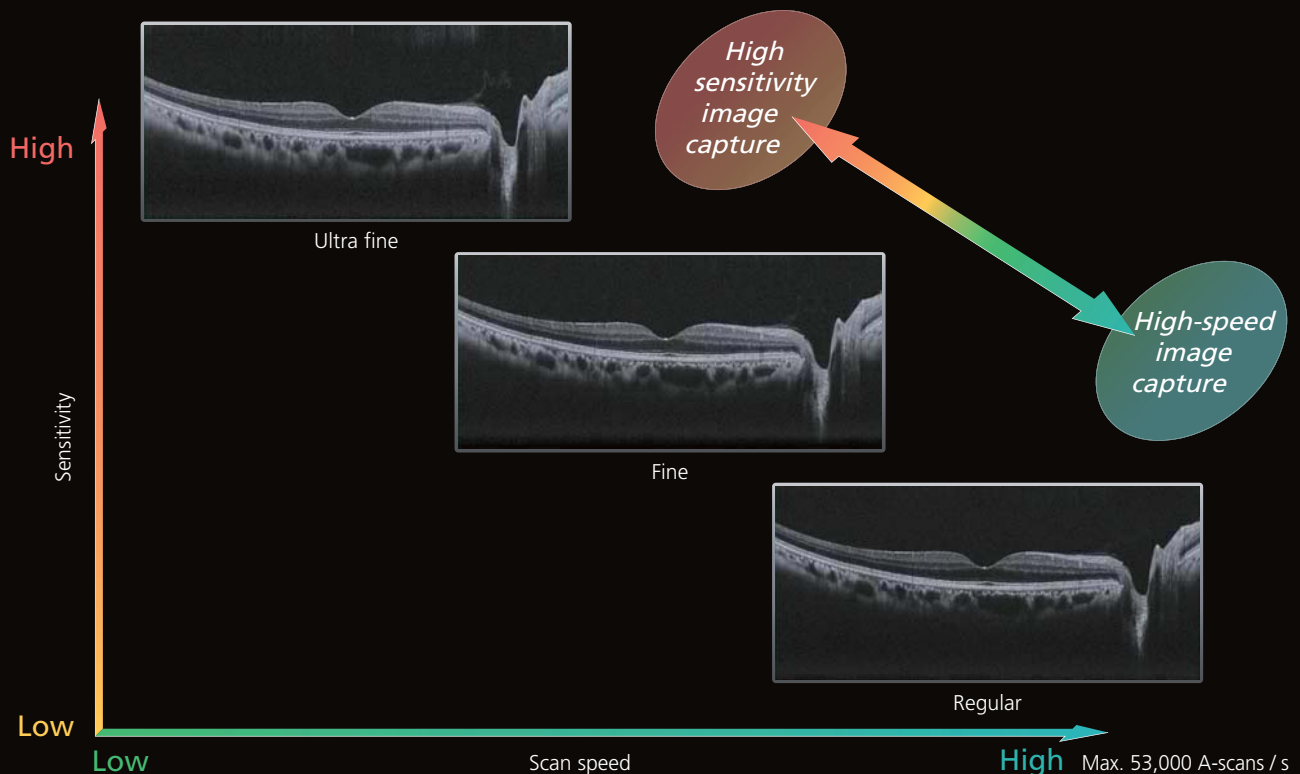


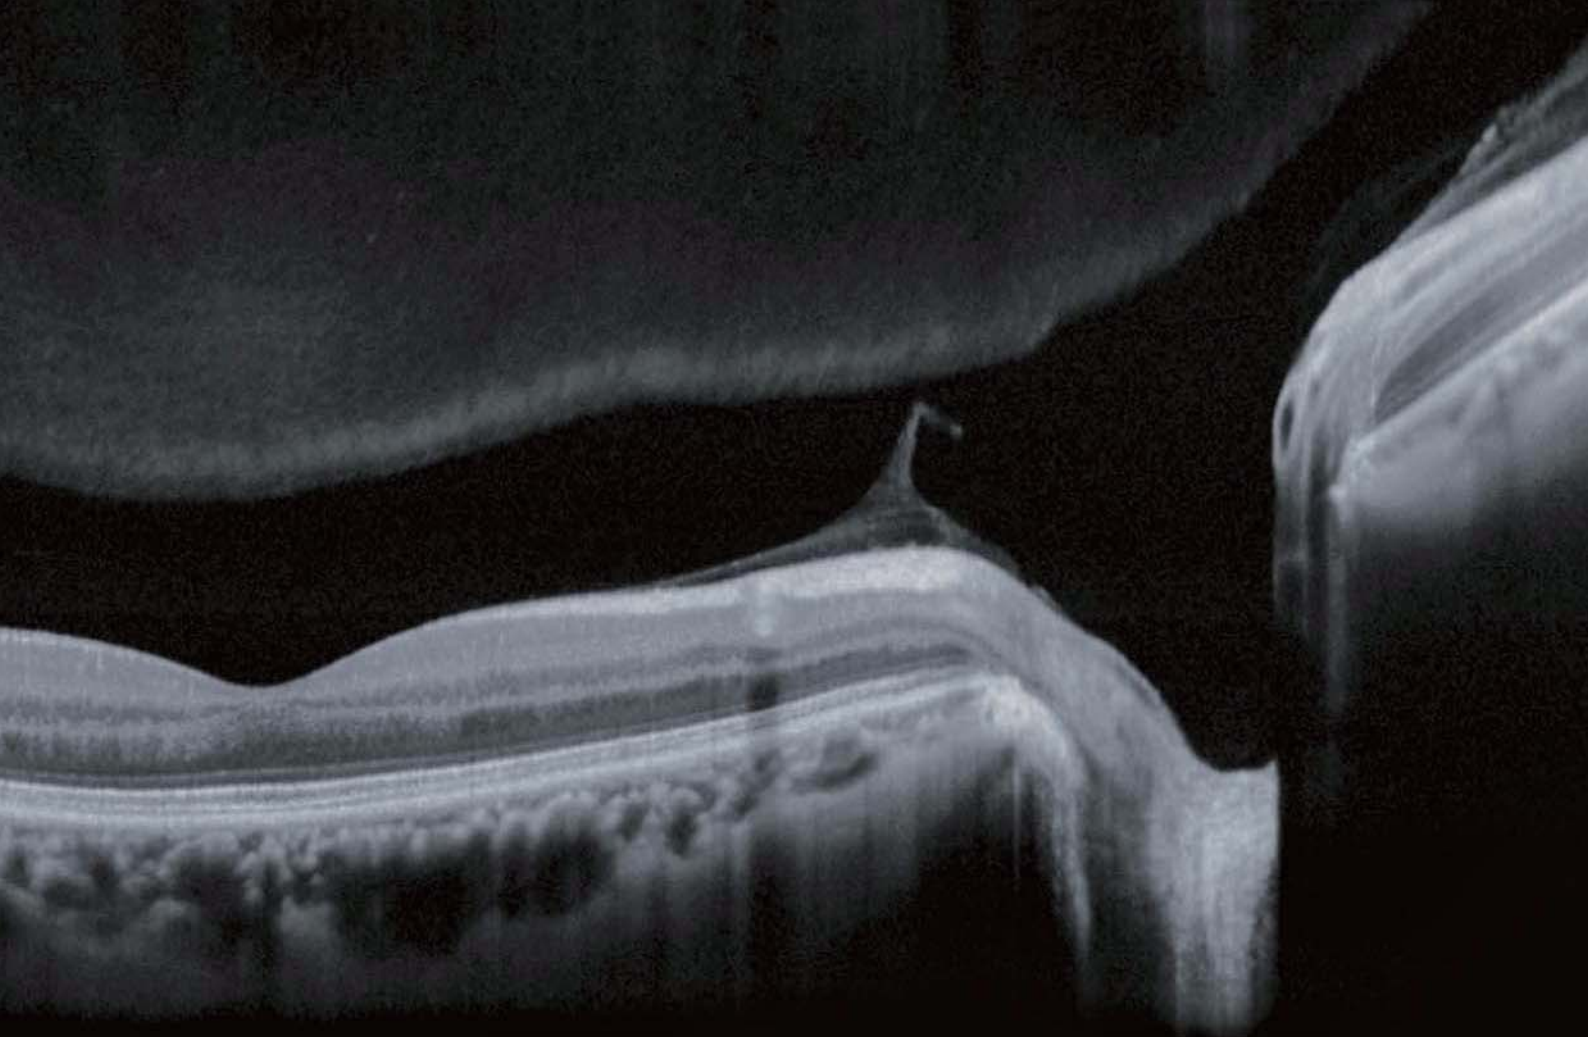


Wide Area Scan 12 x 9

A 12 x 9 mm* wide area image centering around the macula can be captured with the RS-3000 Advance.


*The normative database is based on a 9 x 9 mm region.

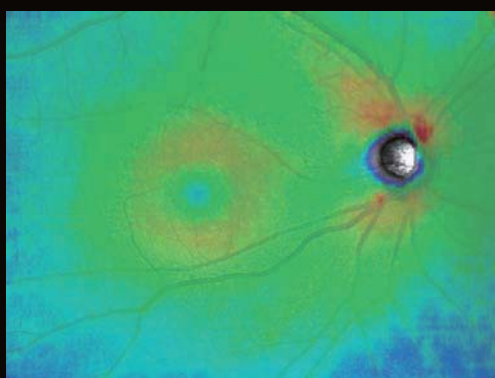


ILM-RPE / BM

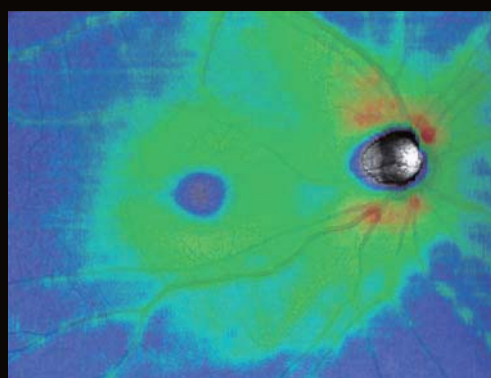

ILM-IPL / INL



ILM-NFL / GCL



NFL/GCL-IPL / INL

Tracing HD plus

The tracing HD plus function in the RS-3000 Advance traces involuntary eye movements to maintain the same scan location on the SLO image for accurate image capture. This function allows accurate averaging of up to 120 images.


Macula multi (cross)



The macula multi scan pattern captures 5 cross-sectional images each in the X and Y directions. High-quality images are easily obtained with the tracing HD plus function.



Capture screen

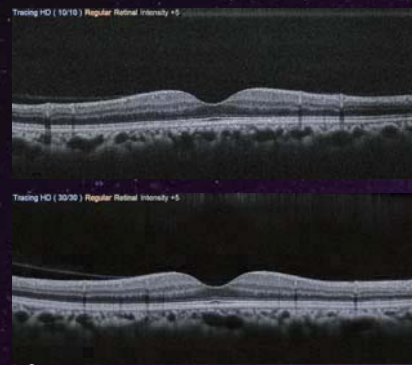

OCT image with averaging of 10* images


*The maximum number of images that could be averaged with previous software.

OCT image with averaging of 30 images


Macula radial and disc radial



The macula radial and disc radial scan patterns capture 6 or 12 radial cross-sectional images centered on the macula and optic disc respectively. The tracing HD plus function ensures the scan is centered on the targeted region.

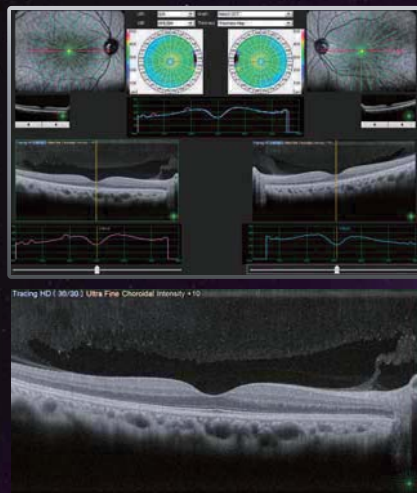


OCT image with averaging of 30 images

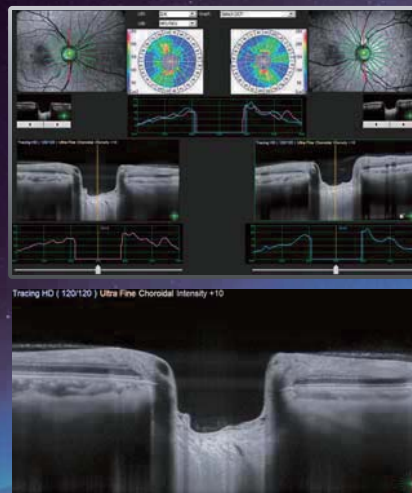


OCT image with averaging of 120 images

HD checker

The HD checker function in the RS-3000 Advance displays the image during averaging and allows an operator to check and finish capturing prior to reaching the number for averaging set by an operator if sufficient image quality is obtained.

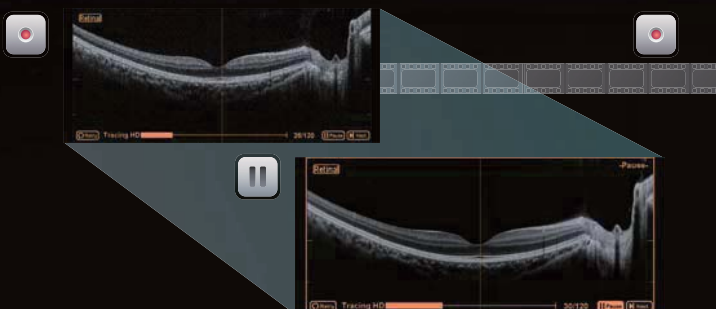

OCT image with averaging of 30 images

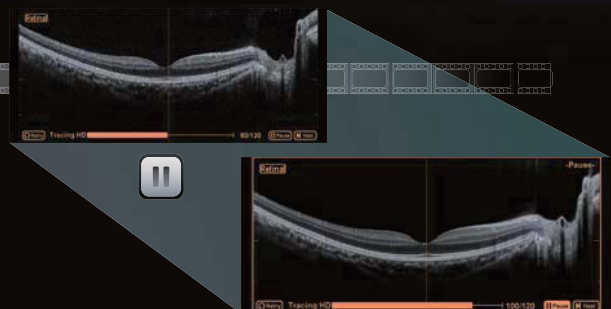

OCT image with averaging of 100 images

Torsion Eye Tracer (TET)


The TET incorporated in the RS-3000 Advance ensures accurate image capture by utilizing fundus information from the high definition SLO image. The three functions, positioning, tracing, and auto shot allow accurate image capture of the targeted region. Ocular cyclotorsion is traced via the torsion correction feature added to the tracing function.

Torsion correction

The torsion correction function ensures the scan is oriented at the right angle even in cases of ocular cyclotorsion and fundus tilt due to head movement or incorrect positioning on the chinrest and forehead rest.



Completion of positioning



Correction of fundus tilt



Positioning

The positioning function briefly provides a still live SLO image in order to easily locate the target of interest on the fundus.







Tracing

The tracing function automatically traces the fundus after positioning is completed. It ensures the scan is centered on the target.



Auto shot


The auto shot function enables automated image capture when the scan is centered on the target and oriented at the right angle. It avoids capturing images in mid-blink or images with incorrect fixation.

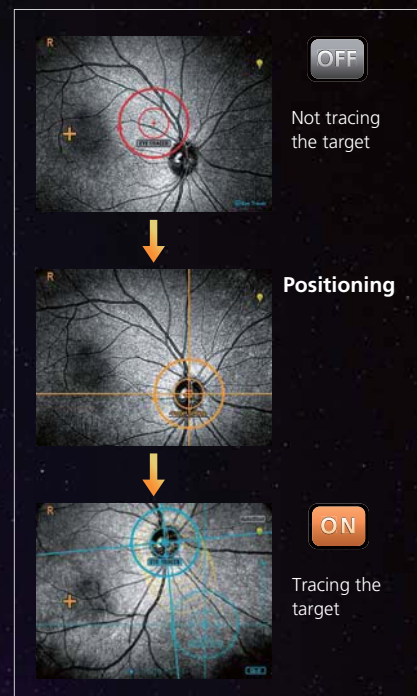


Follow-up Image Capture

The follow-up image capture function in the RS-3000 Advance performs positioning based on the previously captured baseline data, and then tracing and auto shot. It provides ease-of-use and high reproducibility of the image capture for follow-up examination.

The baseline data can be easily registered with one button.



Each baseline image can be displayed in the thumbnail view.



The previously captured position is automatically traced by selecting the registered baseline.




Retina Analysis

Retinal and choroidal modes are available for the RS-3000 Advance and the retinal mode is available for the RS-3000 Lite. The choroidal mode allows a more detailed examination of the choroid.


Macula line with 12 mm horizontal scan



The macula line scan pattern captures a cross-sectional image at a user designated position. The 12 mm horizontal scan of the RS-3000 Advance allows observation of a wide area from the macula to the optic disc in a single image.

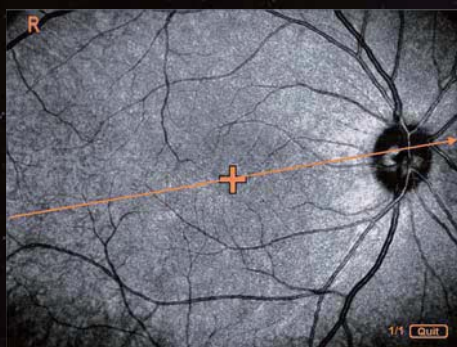


Max. 120
images
averaging

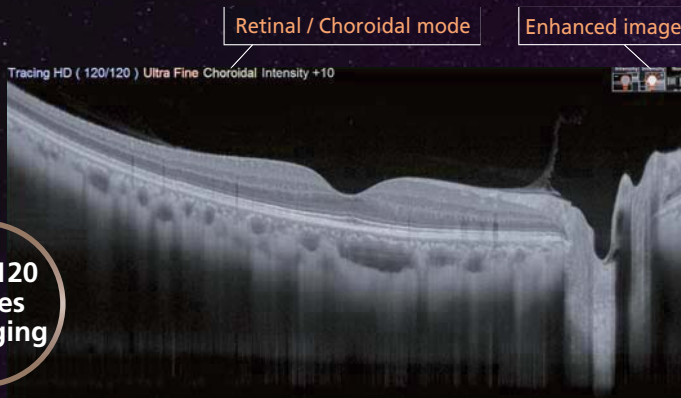


The OCT image with macula line scan pattern clearly shows cross-section of vitreous body, retina, choroid, and optic disc.

Choroidal OCT image (EDI-OCT)

Choroidal mode in the RS-3000 Advance allows capture of highly reflective choroidal images by reversing the image.

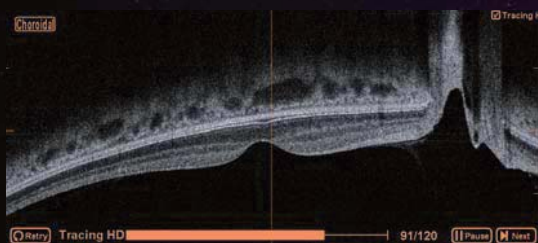

Choroidal OCT image

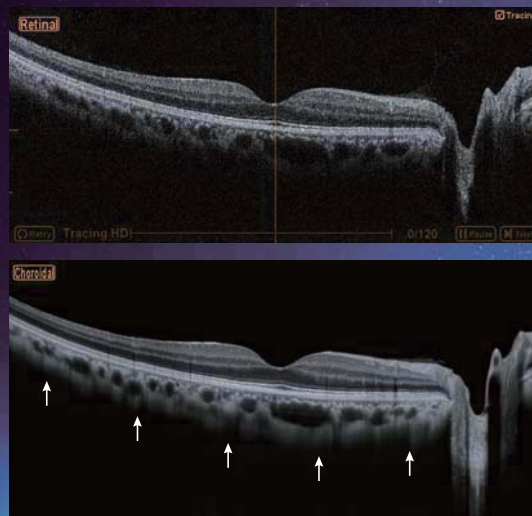


Retinal mode


Choroidal mode

Enhanced image

The enhanced image function allows to adjust bright intensity of an image to enhance details.

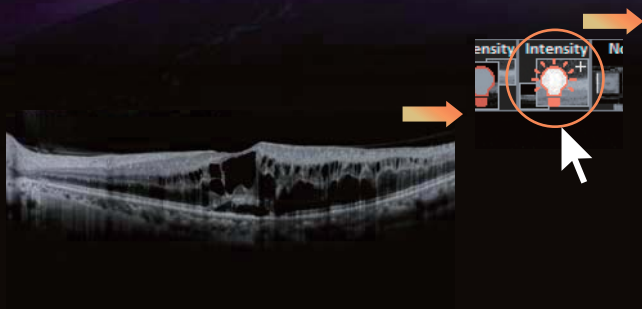


Captured image

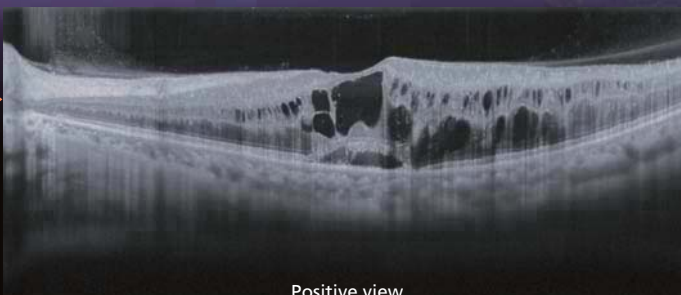

Positive view



Negative view




Color view

Flexible cross scan




The flexible cross scan mode* in the RS-3000 Advance allows free placement of the scan position within a capturing window by shifting the crossing point of the scan pattern lines. This function is useful for capturing an image of pathology that is distant from the center of the SLO image.

*The flexible cross scan mode is available for the macula cross and macula multi (cross) scan patterns.

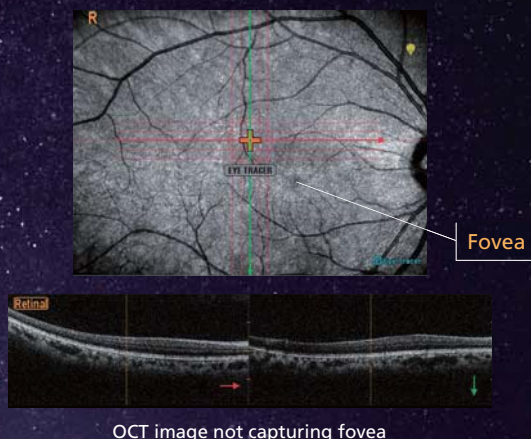

OCT image not capturing fovea

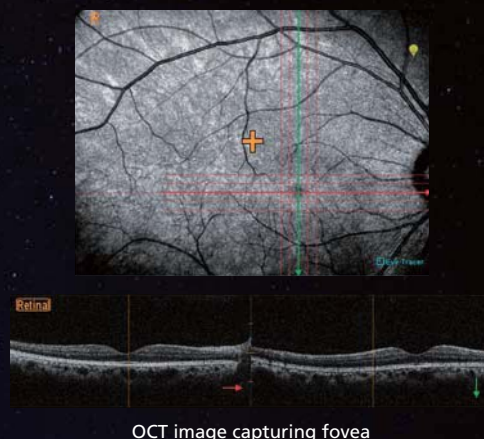


OCT image capturing fovea

Select and Rescan mode (SR mode)

The select and rescan mode in the RS-3000 Advance allows capture of an entire image of the retina with the macula map scan pattern and select a cross-sectional OCT image with the location of lesion from up to 256 images based on user preference. Cross-sectional OCT images can be reacquired on the selected region with the tracing HD plus function. The select and rescan mode is useful in efficiently obtaining a high-quality image of a region of interest.

Macula map scan

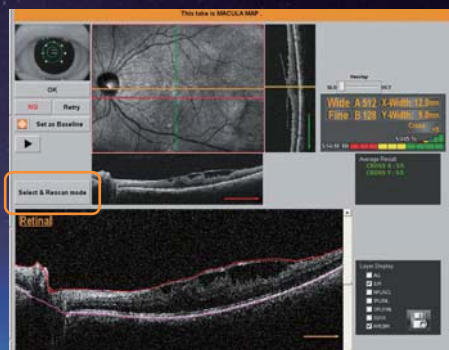

Select an image and then confirm with the select and rescan mode button.




Macula line scan starts on the selected region.

Macula examination

Macula multi (cross)



The macula multi scan pattern enables acquisition of 5 cross-sectional images each in X and Y directions. The appropriate image for diagnosis can be selected from the 10 images.

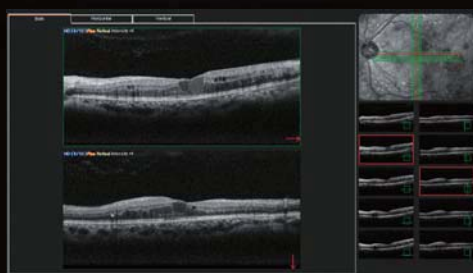


Macula map



The macula map scan pattern captures up to a 12 x 9 mm* area and provides a color-coded map, thickness analysis, surface, and retinal layers.

*12 x 9 mm is available for the RS-3000 Advance.

Analysis chart

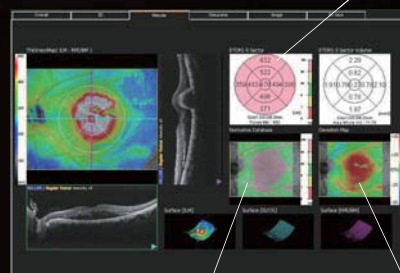


Normative database

Deviation map

Glaucoma Analysis

Wide area scan 12 x 9

Wide area images of 12 x 9 mm centered on the macula can be acquired with the RS-3000 Advance.



Macula map



The glaucoma analysis provides the [NFL+GCL+IPL] analysis, which supplements clinical work-up for the early detection of optic nerve fiber layer defects. The 12 x 9 mm wide area map enables analysis of the [NFL+GCL+IPL] in the peripheral retina.

Analysis display switching tab


[NFL+GCL+IPL]

Color-coded thickness map (12 x 9 mm) of [NFL+GCL+IPL] layers (ILM to IPL / INL) overlaid on SLO or OCT phase fundus image*

*The SLO image is available for the RS-3000 Advance and the OCT phase fundus image is available for the RS-3000 Advance / Lite.

High resolution cross-sectional image display*

*Macula map data and cross-sectional image can be acquired simultaneously with the macula map and macula cross scan patterns.

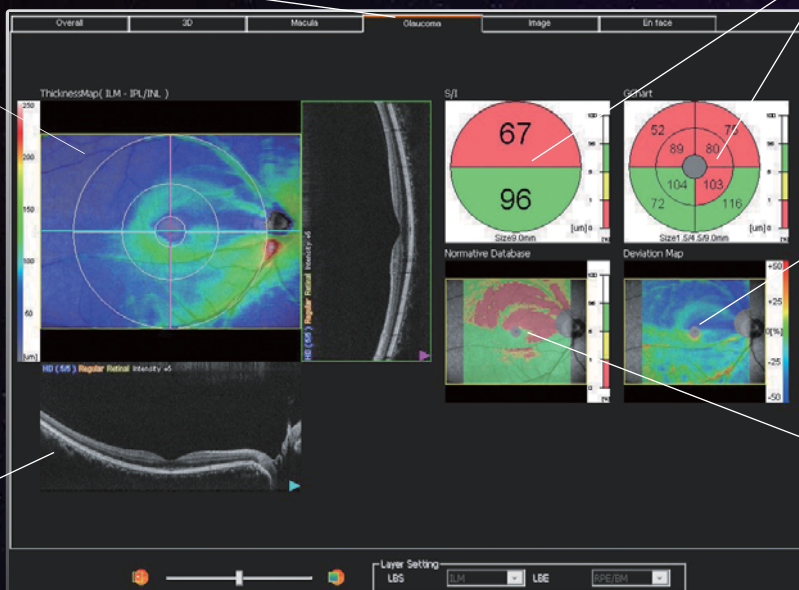

Analysis charts (Superior / Inferior pole, GChart)

Analysis charts of average thickness of each sector surrounding the macula with color code based on comparison to a normative database

Deviation map

Map indicating the deviation, including early variation even within the normal range, from average thickness in a normative database

Normative database*


Color-coded map indicating distribution range of the patient's macular thickness in a population of normal eyes

- More than 95%
- More than 5 to 95%
- More than 1 to 5%
- 0 to 1%


*The normative database is based on a 9 x 9 mm region.

[NFL+GCL+IPL]


The [NFL+GCL+IPL] are layers composed of Nerve Fiber Layer (NFL), Ganglion Cell Layer (GCL), and Inner Plexiform Layer (IPL).

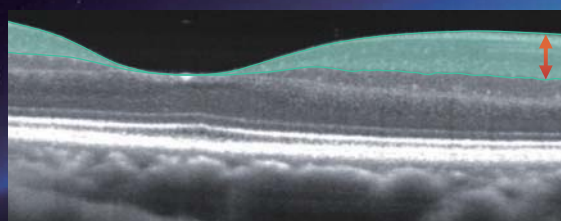

NFL
GCL
IPL



Color fundus photography taken with another device



[NFL+GCL+IPL] thickness map

Disc map



The disc map scan pattern captures an image centered on the disc and provides data for comprehensive disc analysis.

RNFL thickness map

Color-coded thickness map of RNFL layer (ILM to NFL / GCL)

SLO image*


SLO image showing optic disc

TSNIT graph

Graph showing thickness from ILM to NFL / GCL on disc circle with comparison to a normative database

OCT image of disc circle

*The SLO image is available for the RS-3000 Advance and the OCT phase fundus image is available for the RS-3000 Lite.

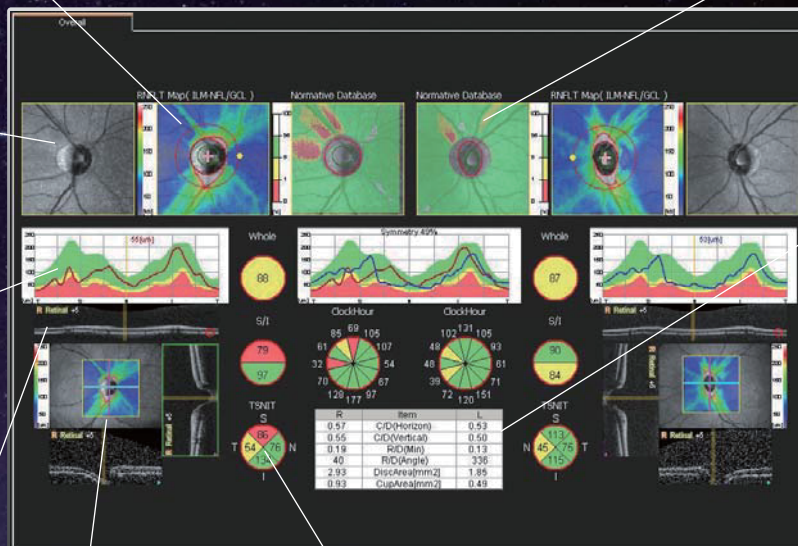

Normative database

Color-coded map indicating distribution range of the patient's RNFL thickness in a population of normal eyes*

*Available for 4.5 x 4.5 mm to 6 x 6 mm area

Analysis table

Table of optic disc analysis
C / D ratio (horizontal)
C / D ratio (vertical)
R / D ratio (minimum)
R / D ratio (angle)
Disc area (mm²)
Cup area (mm²)

Overall tab displaying both right and left eyes

SLO image*

SLO image showing scanned area with color-coded thickness map of user selected layers


Analysis charts

Analysis charts indicating average thickness of Whole, S / I (2-sector), TSNIT (4-sector), and Clock Hour (12-sector), with color code based on comparison to a normative database

Disc circle




The disc circle scan pattern in the RS-3000 Advance captures an image of circle in 3.45 mm diameter centering on the disc and allows RNFL thickness analysis compared to the normative database.

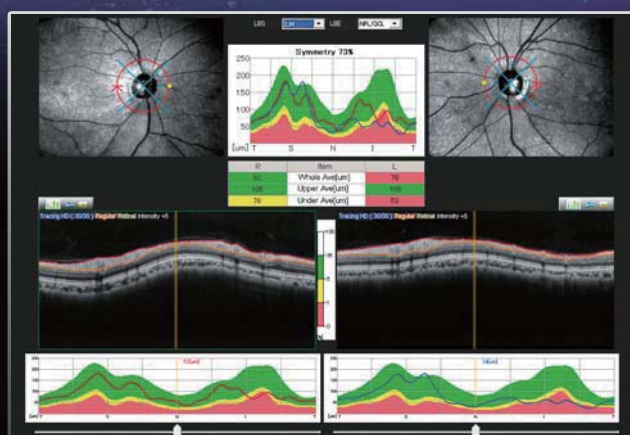

Disc radial



The disc radial scan pattern in the RS-3000 Advance captures 6 or 12 radial cross-sectional images centered on the disc and allows observation of disc shape symmetry.

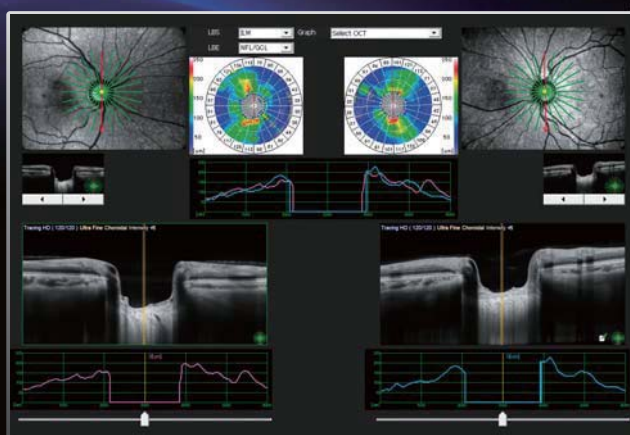

Multifunctional Follow-up

The multifunctional follow-up allows analysis of all the data obtained with the OCT and detailed observation of chronological change in retinal thickness and status. This function displays progression of pathology over the short term, intermediate- and long-term together with a numerical value obtained from RS-3000 Advance / Lite and other examinations such as intraocular pressure and visual field, which provide clinical information for guiding treatment.

Progression mode

The progression mode performs data analysis based on the data captured up to 50 times and displays chronological change in retinal thickness with various maps, charts, and graphs for trend analysis.

Analysis display tab

Progression: Macula / Glaucoma / Custom
Comparison: Macula / Glaucoma

Parameter of the captured data

Date: Capture date (age)
SQL: SLO quality / SSI: OCT quality
Follow-up: Time from the date of baseline data

Map / Data display switching buttons

Anterior segment
SLO or OCT phase
fundus image*
Scan position correction
Color map
Normative database
Deviation map
Difference map

Selection of various parameter sectors

Up to 6 different analyses can be specified.

Graph indicating trend of retinal thickness

Event registration


Treatment record such as start of medication or surgery can be registered and displayed.

Custom registration

Record of the numerical value such as intraocular pressure and visual acuity can be registered and displayed.

Graph analysis of retinal thickness trend

Slope and p-value of each graph

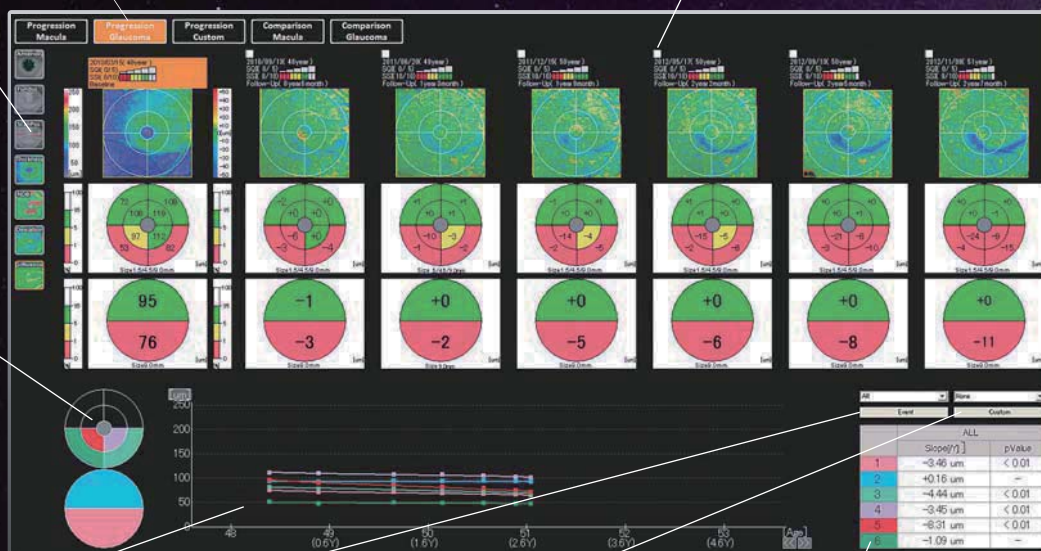

Comparison mode

The comparison mode displays two images selected by the user for comparison and analysis of retinal thickness.

Map / Data display switching buttons

Anterior segment
SLO or OCT phase
fundus image*
Scan position correction

Comparison data


*The SLO image is available for the RS-3000 Advance and the OCT phase fundus image is available for the RS-3000 Advance (macula map, disc map) and RS-3000 Lite.




Graph indicating change in thickness

Glaucoma

The multifunctional follow-up for glaucoma performs data analysis of glaucoma examination based on the data captured up to 50 times and displays trend of chronological change on a graph.

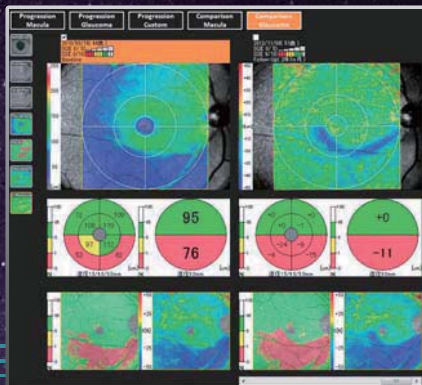


Comparison: Glaucoma (Macula map)

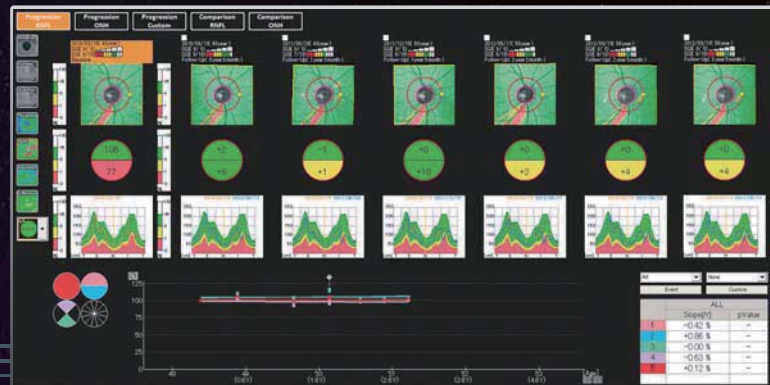


Progression: Glaucoma (Disc map)

Change in [NFL+GCL+IPL] thickness


This function allows the evaluation of the progression of glaucoma in its early stages by displaying changes in retinal thickness compared to the baseline data.

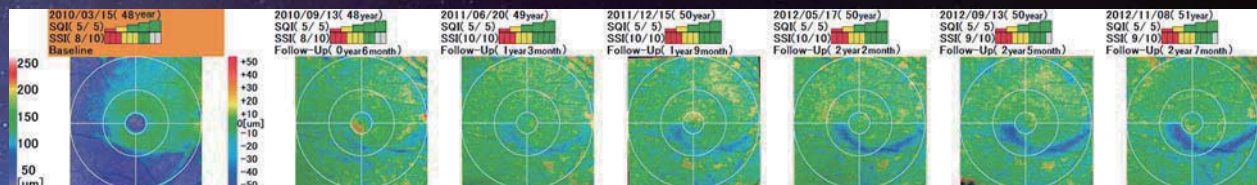


Macula

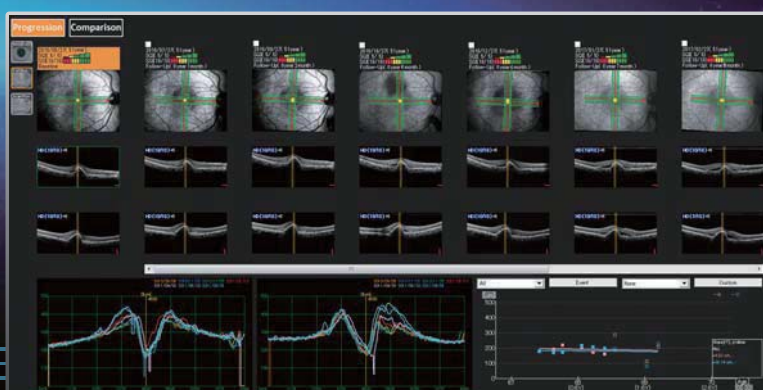

Progression: Macula (Macula multi)

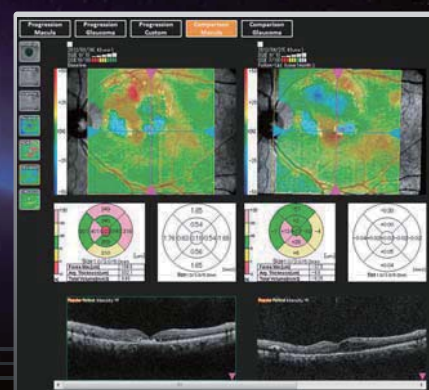

Comparison: Macula (Macula map)

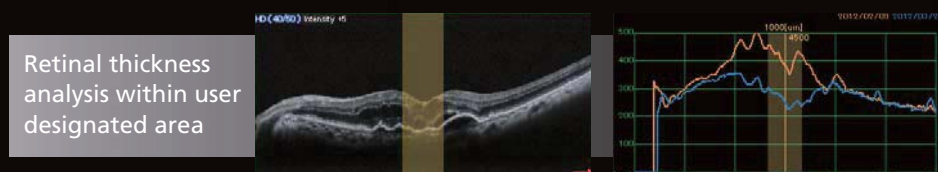


Chronological change in retinal thickness can be analyzed with a graph indicating its trend by designating the area on the thickness graph based on user preference.

Customized Report

The layout of the reports can be customized and the data from separate reports of each scan pattern can be summarized in a single report to avoid printing multiple pages. The report setting can be titled such as glaucoma, macular disease, and screening based on user preference.

Glaucoma

Only the necessary images and analysis results obtained with the macula map (both eyes), disc map (both eyes) are summarized in a report.

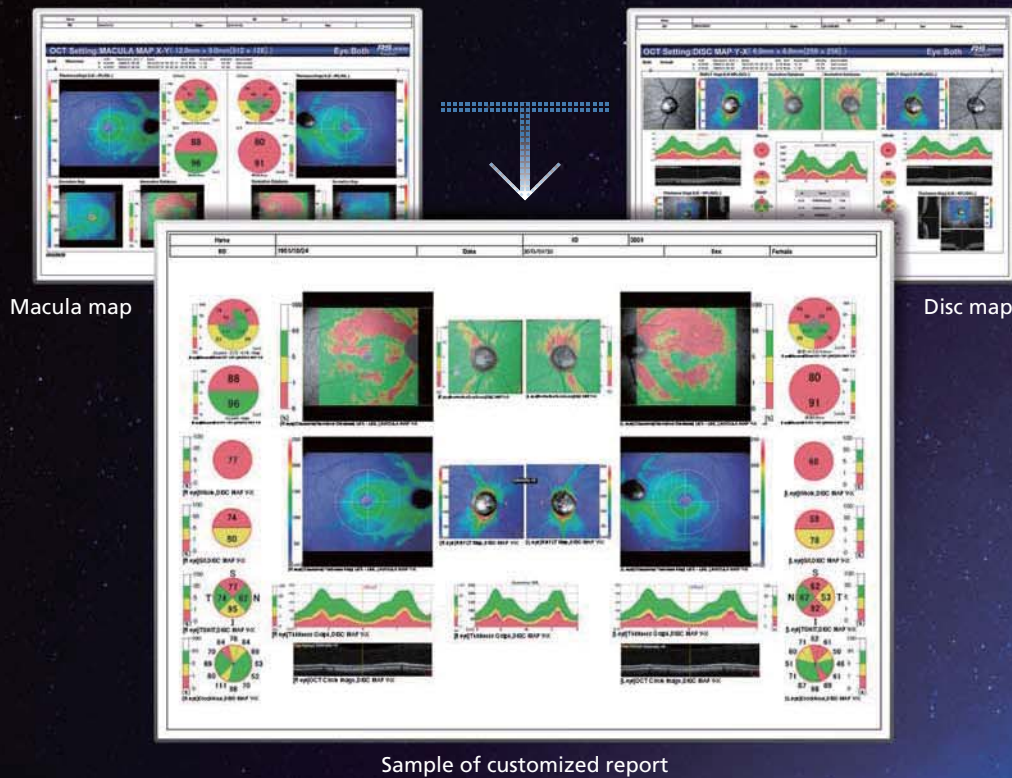

Macula map

- Normative database
- ILM to IPL / INL color map
- GChart, S / I analysis chart

Disc map

- Normative database
- ILM to NFL / GCL color map
- Various analysis charts
- TSNIT graph

Combo release mode

The combo release mode combines scan patterns and facilitates an examination requiring several scan patterns. The scan patterns and their order can be user specified. The scan pattern selected for combo release mode can be preset and reflected on the report.



Default setting

Macula disease



Macula multi



Macula map X-Y

Glaucoma




Macula map Y-X




Disc map Y-X

Macula (one eye)

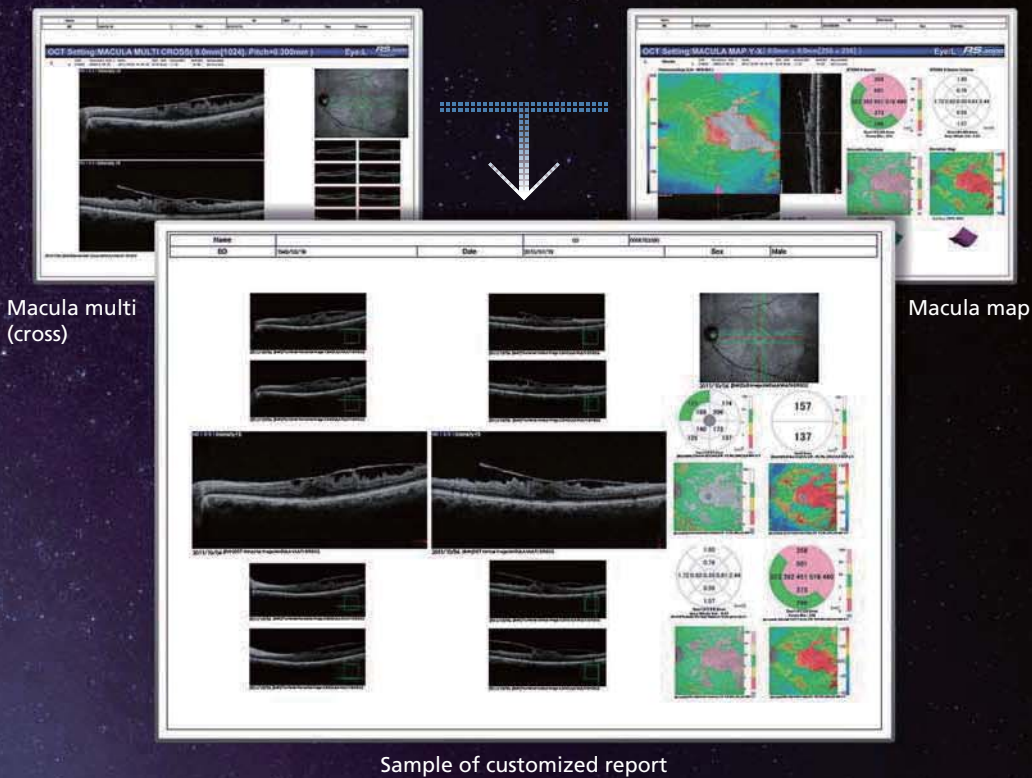


Macula (both eyes)

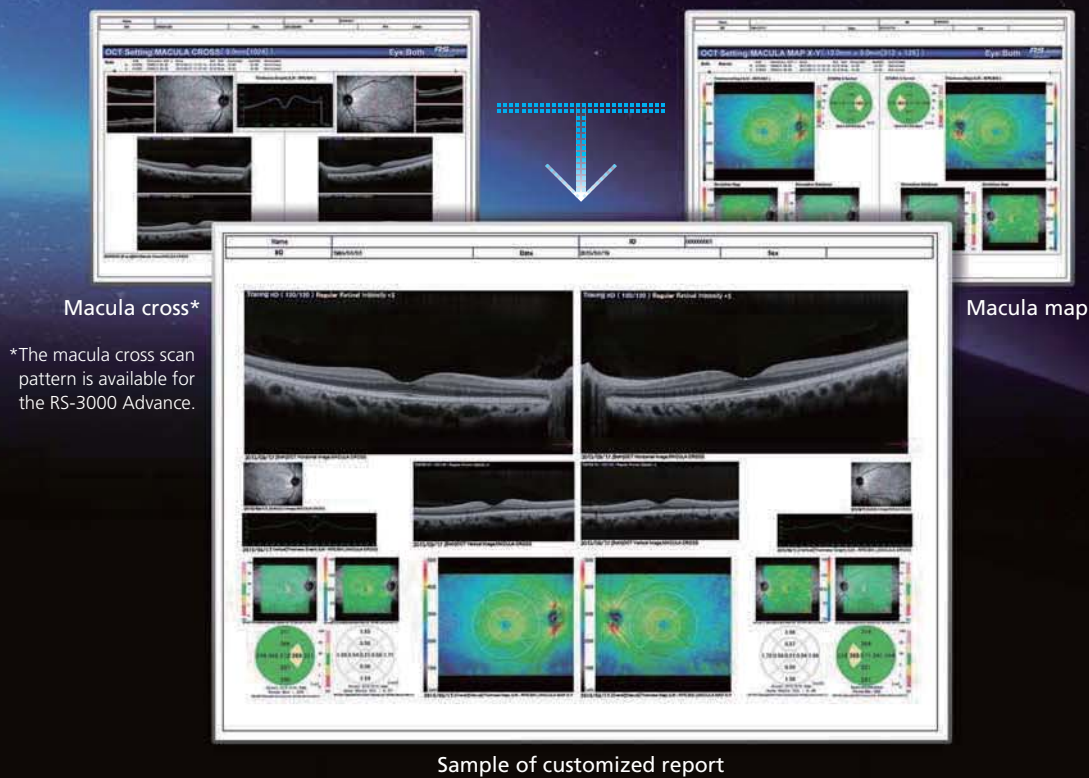

En face OCT

En face OCT imaging is for advanced studies of retinal pathology including factors that compromise photoreceptor function and retinal and choroidal vasculature.

- A. Thickness Map (ILM - RPE / BM)
- B. En face (IPL / INL Offset: +121 μm , Thickness: 42 μm)
- C. B-scan Image
- 1. En face (ILM Offset: 0 μm , Thickness: 42 μm)
- 2. En face (IPL / INL Offset: +21 μm , Thickness: 42 μm)
- 3. En face (RPE / BM Offset: -41 μm , Thickness: 42 μm)
- 4. En face (RPE / BM Offset: 0 μm , Thickness: 125 μm)

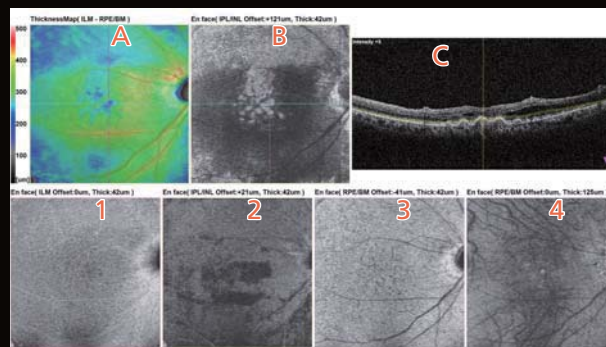


En face OCT Image

NAVIS-EX

NAVIS-EX is an image filing software, which networks the RS-3000 Advance / Lite and other NIDEK fundus imaging devices.


- Analysis and report
- Normative database
- Long axial length normative database (optional software)
- Scalability of connecting with other NIDEK products
- DICOM connectivity

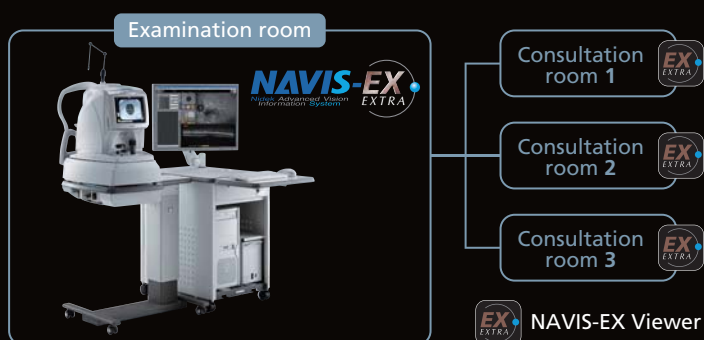

Anterior Segment Analysis

The optional anterior segment module enables observation and analyses of the anterior segment.


Angle measurement




- ACA
Angle between posterior corneal surface and iris surface
- AOD500 (AOD750)
Distance between iris and a point 500 μm (or 750 μm) away from scleral spur on posterior corneal surface
- TISA500 (TISA750)
Area circumscribed with AOD500 (or AOD750) line, posterior corneal surface, line drawn from scleral spur in parallel with AOD line, and iris surface



Cornea measurement




- Corneal thickness
Corneal thickness of apex and user's preferred sites
- Corneal thickness map
Map indicating corneal thickness measured in radial directions




Anterior segment adaptor

The OCT for general screening



Providing the high resolution OCT images and clinically useful analyses, the RS-3000 Lite achieves the optimum balance between cost and performance with its fundus surface imaging system. The RS-3000 Lite has been developed for screening in general eye clinics.

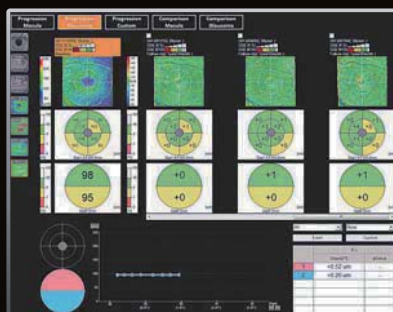

Multifunctional follow-up

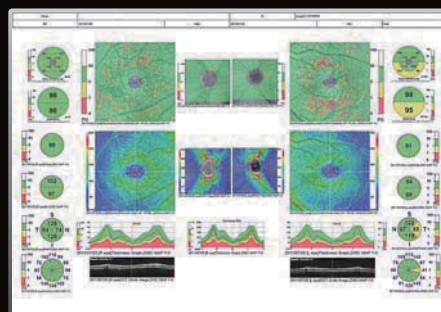

Custom report
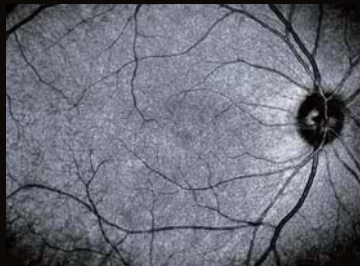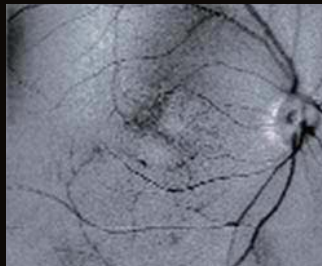
| Model | RS-3000 Advance | RS-3000 Lite |
|--|--|---|
| Fundus surface imaging |  <p>SLO (12 fps frame rate) 40° x 30° angle of view</p> |  <p>OCT phase fundus (1.8 fps frame rate) 36° x 30° angle of view</p> |
| Scan speed | Max. 53,000 A-scans / s | ← |
| OCT sensitivity | Regular, Fine, Ultra fine | Regular, Fine |
| Normative database area | 9 x 9 mm (macula), 6 x 6 mm (disc) | ← |
| Scan pattern (retina) | Macula line (scan angle changeable by 1°) Macula cross Macula map (with cross scan / without cross scan) Macula multi (X-Y: 5 x 5) Macula radial (6 lines / 12 lines) Disc circle Disc map Disc radial (6 lines / 12 lines) | Macula line (scan angle changeable by 15°) Macula map (with cross scan / without cross scan) Macula multi (X-Y: 5 x 5) Disc map |
| Scan pattern (cornea) with optional anterior segment module | Cornea line Cornea cross Cornea radial (6 lines / 12 lines) ACA line | Cornea radial (6 lines / 12 lines) ACA line |
| Image averaging | Max. 120 images | Max. 50 images |
| Choroidal mode | Available | Not available |
| Torsion eye tracer | Available | Not available |
| Follow-up tracing | Available | Not available |
| Follow-up analysis | Available | ← |
| Tracing HD plus | Available | Not available |
| HD checker | Available | Not Available |
| Flexible cross scan | Available | Not Available |
| Select and rescan mode | Available | Not Available |
| Auto shot (for follow-up image capture) | Available | Not available |
| Internal fixation target | Cross shape (laser) | Circle shape (LED) |
| PC monitor | 21" | 17" |

RS-3000 Advance / Lite Specifications

| Model | RS-3000 Advance | RS-3000 Lite |
|---------------------------------------|---|--|
| OCT scanning | | |
| Principle | Spectral domain OCT | ← |
| Optical resolution | Z: 7 µm, X-Y: 20 µm | ← |
| Scan range | X: 3 to 12 mm Y: 3 to 9 mm Z: 2.1 mm | X: 3 to 9 mm Y: 3 to 9 mm Z: 2.1 mm |
| Digital resolution | Z: 4 µm, X-Y: 3 µm | ← |
| OCT light source | SLD, 880 nm | ← |
| Scan speed | Max. 53,000 A-scans / s | ← |
| Acquisition time of 3-D image | 1.6 s in regular mode | ← |
| Internal fixation lamp | 637 nm | 660 nm |
| External fixation lamp | 630 / 565 nm | ← |
| Auto alignment | Z direction | ← |
| Minimum pupil diameter | ø2.5 mm | ← |
| Focus adjustment range | -15 to +10 D (VD=12 mm) | ← |
| Working distance | 35.5 mm | ← |
| Software analysis | Segmentation of 6+1 retinal layers Macular thickness map RNFL thickness map [NFL+GCL+IPL] analysis Optic nerve analysis Follow-up analysis | ← |
| Fundus surface imaging | | |
| Principle | Confocal scanning laser ophthalmoscope (SLO light source: 785 nm) | OCT phase fundus |
| Angle of view | 40° x 30° (zoom: 20° x 15°) | 36° x 30° |
| PC networking | Available | ← |
| Display | Tilttable 8.4-inch color LCD | ← |
| Power supply | AC 100, 120, 230 V 50 / 60 Hz | ← |
| Power consumption | 300 VA | ← |
| Maximum power output (transformer) | 1,000 VA | ← |
| Dimensions / Mass | 380 (W) x 524 (D) x 499 to 531 (H) mm / 34 kg 15.0 (W) x 20.6 (D) x 19.6 to 20.9 (H)" / 75 lbs. | 380 (W) x 524 (D) x 499 to 531 (H) mm / 33 kg 15.0 (W) x 20.6 (D) x 19.6 to 20.9 (H)" / 73 lbs. |

Anterior segment module (optional)


| | |
|-------------------|---|
| Software analysis | Corneal thickness measurement Corneal thickness map Angle measurement |
|-------------------|---|

Motorized optical table (optional)

| | |
|-------------------|--|
| Dimensions / Mass | 639 (W) x 472 (D) x 600 to 850 (H) mm / 28 kg 25.2 (W) x 18.6 (D) x 23.6 to 33.5 (H)" / 62 lbs. |
| Power supply | AC 100 V (available from the transformer) 50 / 60 Hz |
| Power consumption | 150 W |

PC rack (optional)

| | |
|-------------------|---|
| Dimensions / Mass | 620 (W) x 450 (D) x 700 (H) mm / 29 kg 24.4 (W) x 17.7 (D) x 27.6 (H)" / 64 lbs. |
|-------------------|---|

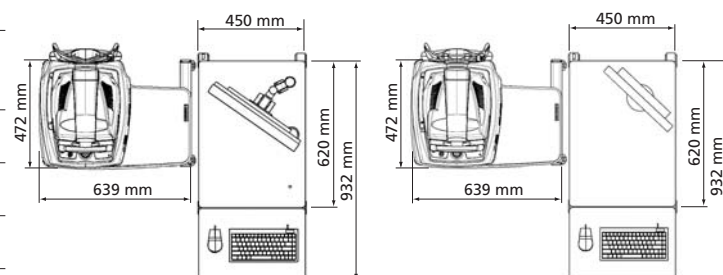

RS-3000 Advance

RS-3000 Lite

Product / Model name: Optical Coherence Tomography RS-3000 Advance / Lite
Listed features in this brochure are intended for non-US practitioners.
Specifications may vary depending on circumstances in each country.
Specifications and design are subject to change without notice.



HEAD OFFICE
(International Div.)
34-14 Maehama, Hiroishi
Gamagori, Aichi 443-0038,
Japan
TEL: +81-533-67-8895
URL: <http://www.nidek.co.jp>
[Manufacturer]

TOKYO OFFICE
(International Div.)
3F Sumitomo Fudosan Hongo
Bldg., 3-22-5 Hongo, Bunkyo-ku,
Tokyo 113-0033, Japan
TEL: +81-3-5844-2641
URL: <http://www.nidek.com>

NIDEK INC.
47651 Westinghouse Drive
Fremont, CA 94539, U.S.A.
TEL: +1-510-226-5700
+1-800-223-9044
(US only)
URL: <http://usa.nidek.com>

NIDEK S.A.
Europarc
13, rue Auguste Perret
94042 Créteil, France
TEL: +33-1-49 80 97 97
URL: <http://www.nidek.fr>

NIDEK TECHNOLOGIES Srl
Via dell'Artigianato,
6 / A 35020 Albignasego
(Padova), Italy
TEL: +39 049 8629200 / 8626399
URL: <http://www.nidektechnologies.it>

NIDEK (SHANGHAI) CO., LTD.
Rm 915, China Venturetech
Plaza, No.819 Nanjing West Rd,
Jing An District, Shanghai
China 200041
TEL: +86 021-5212-7942
URL: <http://www.nidek-china.cn>

NIDEK SINGAPORE PTE. LTD.
51 Changi Business Park
Central 2 #06-14
The Signature Singapore
486066
TEL: +65 6588 0389

